Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

Guangzhou Hulian Beauty Equipment Co.,Ltd

Slimming & Facial beauty machine
* Cavitation
* Cooling Therapy +LED
* Tri-polar RF with photon for facial
* Bi-polar for eyes

BR 8.0 P USER'S MANUAL

Cavitation + Cooling + RF SYSTEM

Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

Warning

Honorable Clients

Thanks for your attention to our products BR8.0P Cavitation Multifunction System.

For better using this machine, please read through the user manual and follow the instructions carefully when you operate the machine.

It forbids someone to open and remove the mainframe of this machine unless authorized from the our original manufacturer.

Please contact us in time if there is any question during operation.

Professional technique we made, just to satisfy your kinds of requirements in a good way.

Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

CONTENTS

- Parts introduction ----------3
- Introduction ---------- 5
- Functions and Operation----------6
- Notice ----------11
- Forbidden group ----------12
- Maintenance ----------12
- Technical parameters ----------14
- Annex List ----------15

Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

Parts Information

Accessories

40KHz Cavitation

Cryo+ Led Head

Tri-polar RF head

Bi-polar RF Head

Handle Support Shelf

Power line

Inner Hexagon Screw

Screw Driver

Installation

First: Connect the handles according to the Roman Numerals.

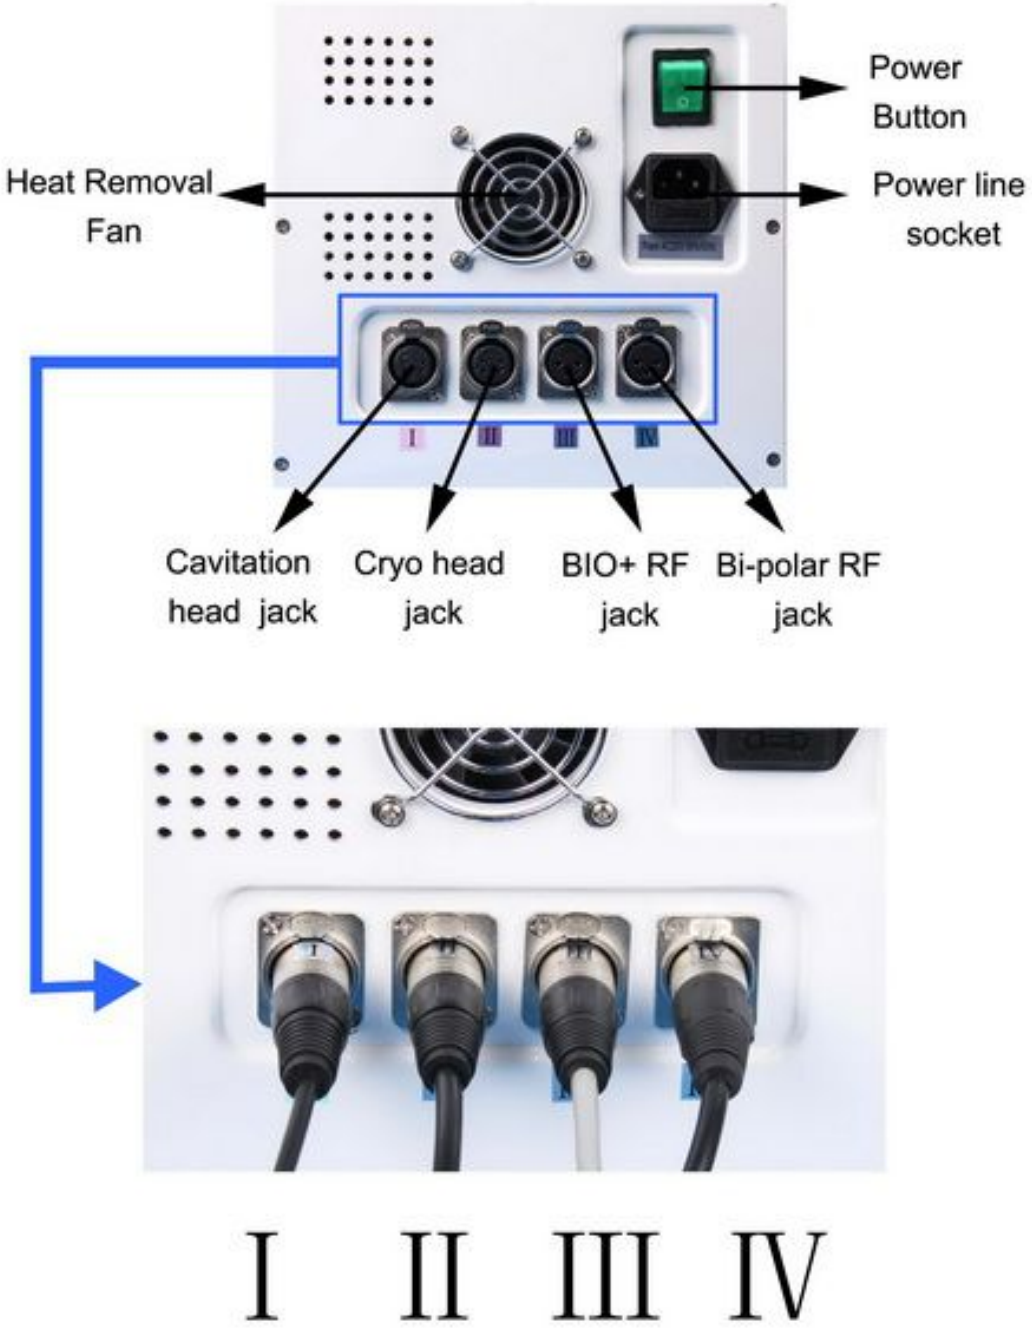

Second: Connect the Power line and press the power button to test the machine.

Introduction

Cavitation with red LED therapy

Can promote tissue metabolism, repel the cellulite, tighten the skin, strengthen the skin elasticity and so on. Its effect will last for a long time. Meanwhile, it can enhance the elasticity of muscle and improve the metabolism of cells.

With collective strong sound wave head, strong sound wave of 40KHZ may be emitted to human body for impacting fat cells fiercely and causing friction motion between fat cells. This may cause effective consumption of calories and moisture in fat cells and reduce the size of fat cells. What's more, sound wave vibration may cause fierce impact of fat cells to make them be exploded instantaneously to reduce the amount of fat cells and thereby achieve the effects of removing fat.

Facial Bipolar RF

A capacitive coupling electrode is used for transmitting radio-wave energy and generating an electric field for entering into subcutaneous tissue through the skin surface. In the high-frequency of 450khz, this electric field changes its polarity for 450,000 times per second. To reply to the rapid change in electrode, directions of electrical particles the skin are also changed.

By this time, natural electric resistance in the subcutaneous tissue moves and generates heat energy. As the papillary dermis collagen may immediately shrink when the temperature is within the range from 60 to 70 Centigrade, after wrinkle treatment, client may immediately sense the skin tightening effects as it is being lifted and firmed.

BIO & RF

Eliminate black circles, promote the ocular region blood circulation effectively, increase the product absorbing.

Stick to enhance rejuvenation: use of positive and negative micro-current activation energy release skin cells, so that rapid synthesis of fibroblasts collagen, elastic skin revert to the original compact, the skin causing the skin to stimulate the muscle tension is increased, thereby gradually eliminate wrinkles, prevent skin aging, restoring skin elasticity, facial improvement.

Cryo head with LED

The physical effects and the results of 5 centigrade:
1. Constricting blood vessels and pores. If it is also an enormous result for reducing rough pores.
2. To strengthen collagen, upgrade to more elastic and well-order skin, and remove the fine line and wrinkles.
3. To constrict blood vessels, reduce dilated veins effectively and the appearance of red tendons, and filter poisonous waste in the veins. It is also good for even the skin tone and blotches.
4. Decreasing the metabolic rate, cell activities, sensitivities of neurons, and reducing reddish look of swollen on skin, pain of swelling, especially for sensitive skin.

Functions and Operation

Preparation Before Use

1. Install the power line on the machine, put the handle-pieces into the corresponding racks.

2. Check the host power cable is connected.

User Interface

Press any key to enter the main menu to enter the system.
Choose the right function according to requirement.

40KHz Cavitation+led

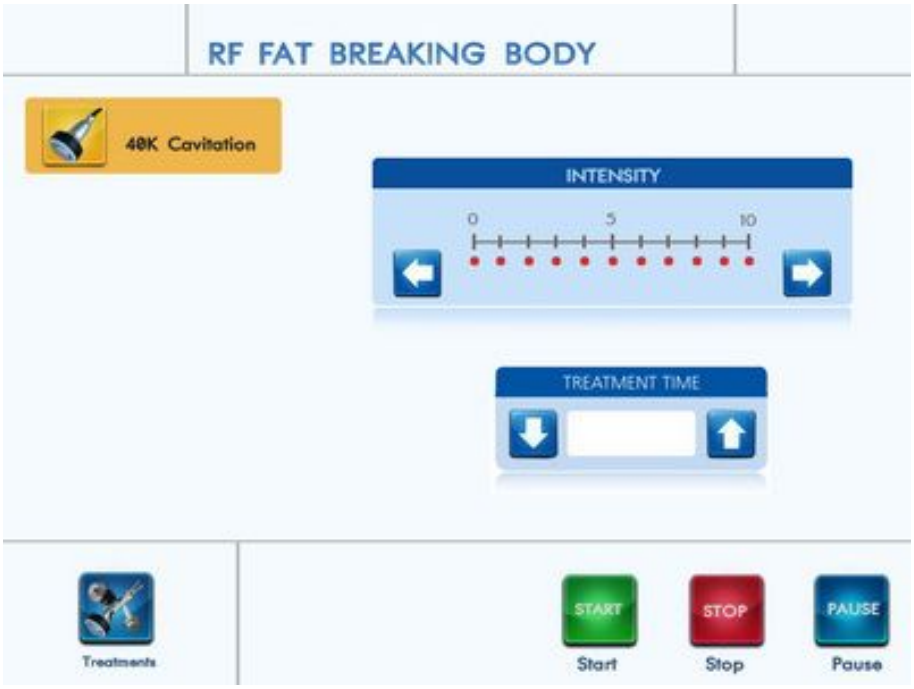

①. Click [1] and choose "Cavitation" ,enter the interface of Cavitation.

②. Click to adjust the working time ,set the working time about 20

minutes.

③. Click to set the working intensity : 1 (weak) ~ 10 (strong)

④.Applied gel on fleshy parts(eg.abdomen,hip,thigh) The amount depends on moving flexibility of the ultrasonic slimming head.

⑤.click start/pause . the machine will start working
⑥.Beautician hold the ultrasound head to move slowly on skin, in circle or beeline repeatedly, the other hand push the fat towards the ultrasonic cavitation slimming head.
⑦.Do not use on back, avoid using on bones.
⑧.Do not use on uterus part when women do abdomen care.Abdomen treatment during menstruate should be avoided.
⑨.The machine will pause automatically if the setting time is over.
⑩.Clean the leftovers with hot towel, use warm towel to clean the ultrasonic cavitation slimming head.

Do as following ways to treat on the body:

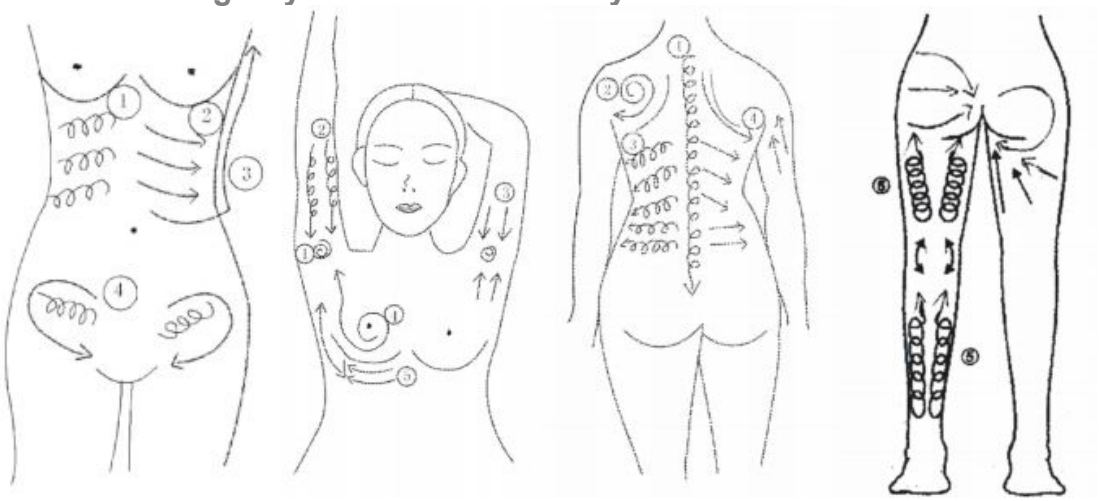

Bi-polar RF

Hulian Beauty Equipment Company			
Contact:	Leo	Tel: +86 20 89095112	Mobil: +86 18825145209
Email:	hulianleo@gmail.com	Website:	www.hulian.en.alibaba.com
Address:	No.9018 Xingdu Hotel Changgang middle road, Haizhu Guangzhou Guangdong,China		

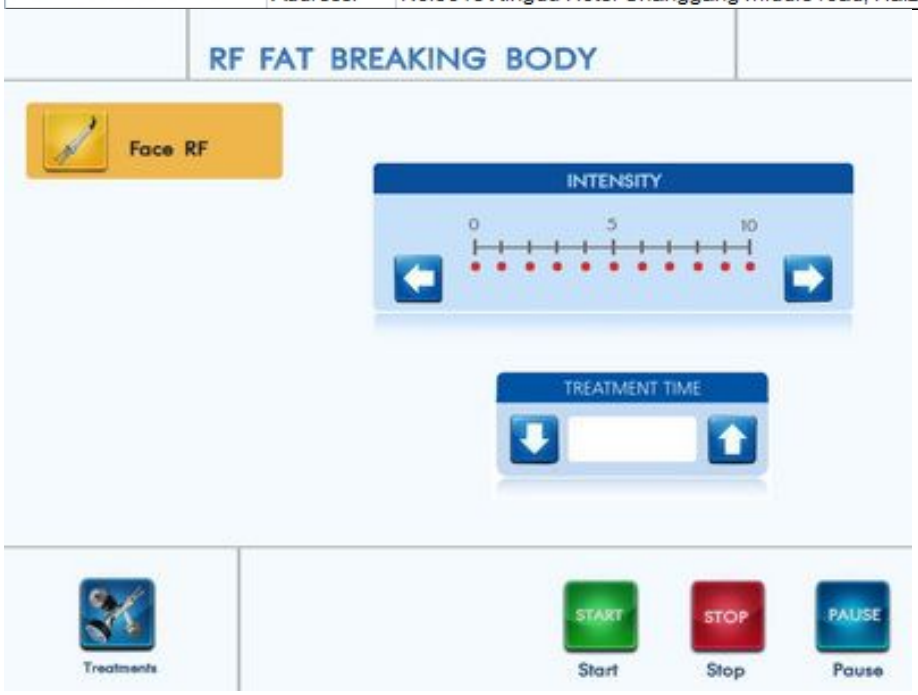

①Click [1] and choose "RF" ,enter the interface of RF .

②click click to adjust the working time ,set the working time about 20 minutes,

③Click to set the working intensity : 1 (weak) ~ 10 (strong)

④.Applied gel on the treatment skin,,click start/pause . the machine will start working.

⑤the Beautician move handle in circle, the electrode probe move from inside out,operating on both side,right and left, one side over to start to other side, and must lower the intensity accordingly as less fat on forehead and eyes.do not let gel into eyes,do not stay unmoved.

⑥.The machine will pause automatically if the setting time is over.

⑦.Clean the leftovers with hot towel, use warm towel to clean handle

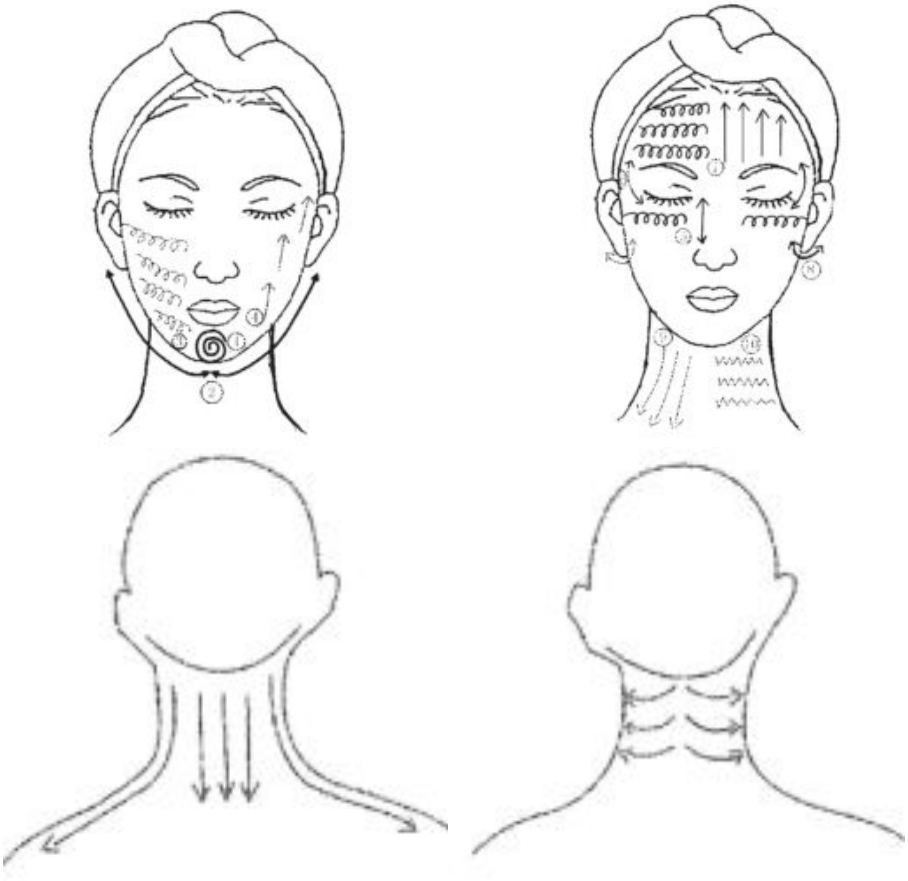

BIO + RF (BIO micro current)

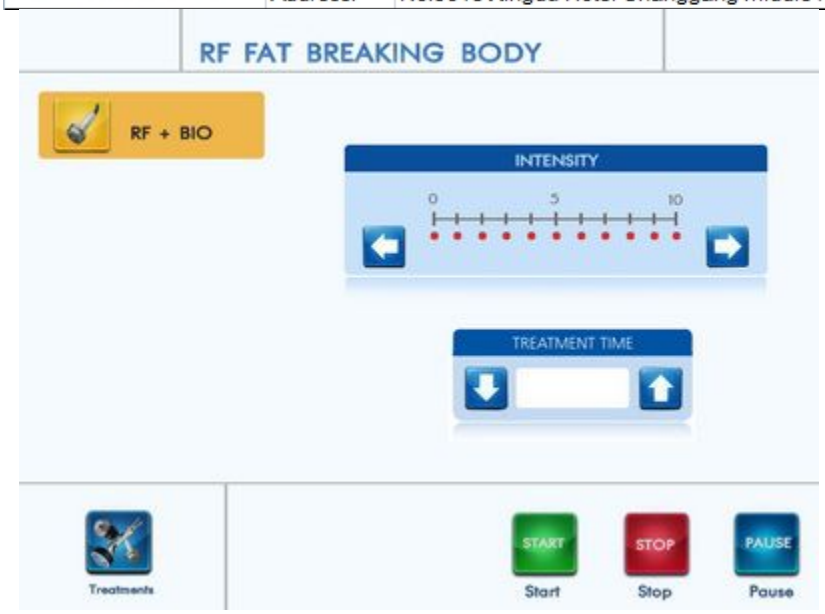

①.Click [1] and choose "RF" , enter the interface of BIO+RF.

②.Click to adjust the working time ,set the working time about 20 minutes,

③.Click to set the working intensity : 1 (weak) ~ 10 (strong)

④.Applied gel on the treatment skin, click START/PAUSE and the machine will start working.

⑤.The beautician move handle in circle, the electrode probe move from inside to out, operating on both sides, right and left, one side over to start to other side, and must lower the intensity accordingly as less fat on forehead and eyes. Do not let gel into eyes, do not stay unmoved.

⑥.The machine will pause automatically if the setting time is over.

⑦.Clean the leftovers with hot towel, use warm towel to clean handle.

Cryo + LED

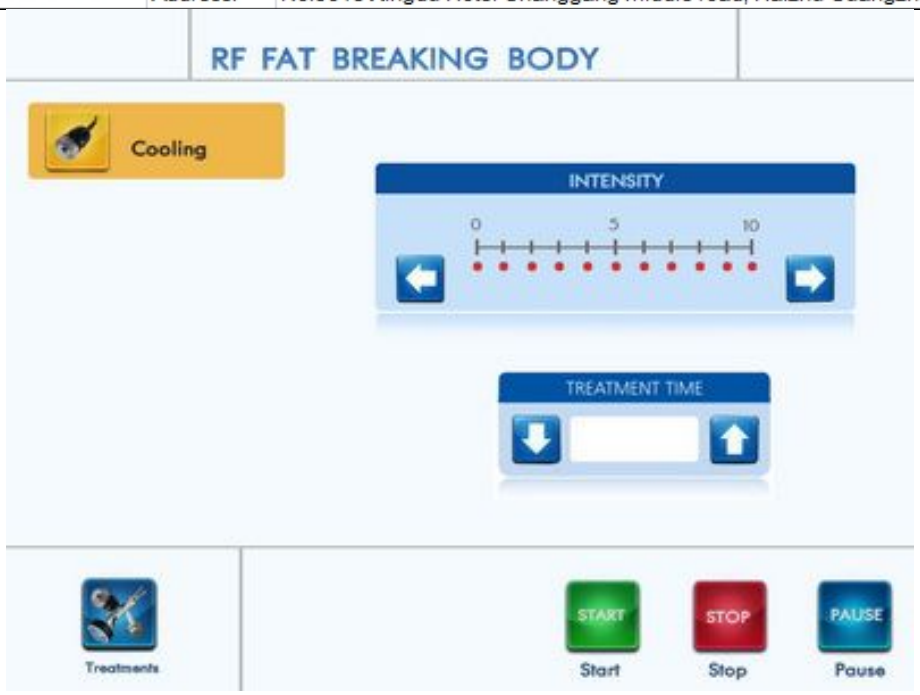

①.Click [1] and choose "cooling" , enter the interface of cooling .

②. Click to adjust the working time ,set the working time about 20 minutes.

③.Click to set the working intensity : 1 (weak) ~ 10 (strong).

④.Applied gel on the treatment skin,click start/pause ,the machine will start working.

⑤.Move the handle on skin slowly,do not stay unmoved.

⑥.The machine will pause automatically if the setting time is over.

⑦.Clean the leftovers with hot towel, use warm towel to clean handle.

Notice

1. Before operation, please use sufficient gel for better effects.
2.The ultrasound head should not stay out of work for too long time while out putting energy, do not use it on bones. Click “PAUSE” to stop working to avoid damage.
3. BIO head should not stay still at one part for too long time.
4. Do not use on eyeball top, Adam's apple,heart .Do not stay still on one part for too long.

Forbidden group

1.People who has fever, infectious diseases, acute diseases.
2. People with heart disease or configured cardiac pacemaker.
3. Patients with severe high blood pressure, tumor disease, asthma, deep vein thrombosis,Varix, thyroid ,cancer, falling sickness.
4. People with hemorrhagic disease, trauma, vascular rupture, skin inflammation, skin disease.
5.Pregnant women.
6. Do not use at the abdomen during menstrual period.
7. Medical Plastic parts, or parts with metal inside.
8. People with an abnormal immune system.

Maintenance

This chapter describes how to use and maintain the system including precautionary maintenance, ordinary maintenance, and extraordinary maintenance and also describes some malfunctions and solutions.

The customer can carry out the maintenance through the measurements listed in this chapter. Maintenance and any other work can only be performed by authorized professionals.

WARNING

Before any maintenance work turn the power off and unplug device. Failure to turn off the power may cause an electric shock, damage to the device and bodily injury. Never attempt to remove the back panel or device casing. Unauthorized tampering with the devices internal system will automatically void the warranty.

1. Warranty

1. Three months for handle-pieces and one year from the host of the machine from the date of original purchase.

2. Manufacturer won't bear any responsibility:

A. Damage caused by accident, abuse, misuse or misapplication, it will be repaired with repair fee.

B. Damage caused by service performed by anyone who is not technician or qualified by manufacturer.

C. The product or part that has been modified without any permission of manufacturer.

2.Ordinary Maintenance

The operator has to check in time the wear of the accessory parts (for instance line cords, electrodes, etc), arranging for their substitution at the right moment, if it is necessary.

3. Extraordinary Maintenance

The interventions of extraordinary maintenance have to be done by the qualified staff, trained an authorized by BEIR.

4.Maintenance by the Operator

Trained and authorized hospital personnel can carry out routine maintenance work. Authorized persons are exclusively persons who have been trained by BEIR .The following routine maintenance work must be carried out:

Routine Maintenance Work

Maintenance work	interval
Check and clean outside surface	Daily, before/after use
Check, disinfect and sterilize accessories & transducer which connected to the patient	daily
Check the hand-piece plugs & hoses	daily

5. System Trouble Shooting

This section lists some malfunction phenomenon and solutions.

Malfunction phenomenon	Solutions
While touching the button on the screen, the system has no reaction	Please contact the dealer.
There is no power delivery on the Cavitation treatment head	Don't trigger "READY" on the screen. Be sure away from direct solar radiation or high frequency radiation. Defective ultrasonic generator module.
	Please contact the dealer.
Malfunction of RF energy output on the treatment head	Don't trigger "START" on the screen. Re-install the tip firmly. Be sure away from direct solar radiation or high frequency radiation.
Insufficient power of Ultrasound	Defective ultrasonic treatment hand-piece or the service life of cavitation head had been executed over 300 hours. Contact the dealer.

Parameter

Output Power	≤ 50 W
Display	8 inch color touch screen
Frequency	40KHz 25W-50W deepest fat
RF frequency:	5Mhz for Facial
BIO	skin beauty and cosmetics permeation
Cryo degree	from 3℃ to 8 ℃ for skin tighten and facial slimming
Wave Length	Red light: 630nm
	Yellow light : 577nm-597nm
	Green light: 492nm-576nm
	Blue Light: 455nm-492nm
Power:	150W
Voltage	110-230V/50/60Hz
MEAS	50CM*45CM*40CM

GW/NW:	12KG, 7KG

Annex List

Item	Part name	Quantity
1	Mainframe	1set
2	Power supply line	1pc
3	Use manual	1copy
4	40K Cavitation head	1pc
5	Bi-polar RF head	1pc
6	BIO handle	1pc
7	Cryo led handle	1pc
8	Annex shelf	1pc
9	10A fuse	2pcs
10	Inner hexagon screw	2pcs
11	Inner hexagon screw driver	1pc